

viewLinc Alarm Report

Alarm events from 2012-11-18 12:31:45 to 2012-11-19 12:31:45
 Report generated on 2012-11-19 12:32:14 (UTC-08:00) Pacific Time (US & Canada)
 Include zones and locations: All Locations
 Include alarm details: Yes


Summary

Total active alarms: 12
Activated alarms: 9
Deactivated alarms: 7
Acknowledged alarms: 0

Activation	Deactivation	Duration	Source	Description	Acknowledgement
2012-11-11 11:10:00		8 days, 1 hour, 22 minutes, 14 seconds	Threshold Alarm: Default Threshold Alarm for Threshold: location value greater than 20.00 C for System/Lab Area 2/Zone D/Location D Temp	Threshold Alarm: Default Threshold Alarm for Threshold: location value greater than 20.00 C for System/Lab Area 2/Zone D/Location D Temp Affected location: System/Lab Area 2/Zone D/Location D Temp (25306)	
Details:					
2012-11-11 11:10:00		Activating alarm.			
2012-11-15 05:37:41		4 days, 6 hours, 54 minutes, 32 seconds	Device Device B (04122204) on Host viewlincServer	Device Configuration Alarm: Custom Alarm for Device Device B (04122204) on Host viewlincServer Affected locations: Location D Temp (25306),Location D %RH (25304)	
Details:					
2012-11-15 05:37:41		Activating alarm.			
2012-11-18 12:08:46	2012-11-18 12:31:46	23 minutes	Device Device A (07024034) on Host viewlincServer	Device Configuration Alarm: Default Logger Configuration Alarm for Device Device A (07024034) on Host viewlincServer Affected locations: pPRESSUREtEST (36915),Temperature (36917)	
Details:					
2012-11-18 12:08:46		Activating alarm.			
2012-11-18 12:31:46		Alarm condition no longer met. Deactivating alarm.			

viewLinc Location History Report

Location history	from 2012-11-18 12:39:23 to 2012-11-19 12:39:23
Report generated on	2012-11-19 12:39:24 (UTC-08:00) Pacific Time (US & Canada)
Include trend graphs:	Yes
Include threshold lines on graphs:	Yes
Include zones and locations:	System/Zone P
Include report summary tables:	Yes
Include device samples:	No
Include real-time values:	No
Include statistics tables:	No
Include summary statistics:	Yes
Include interval statistics tables:	No
Include interval statistics graphs:	No

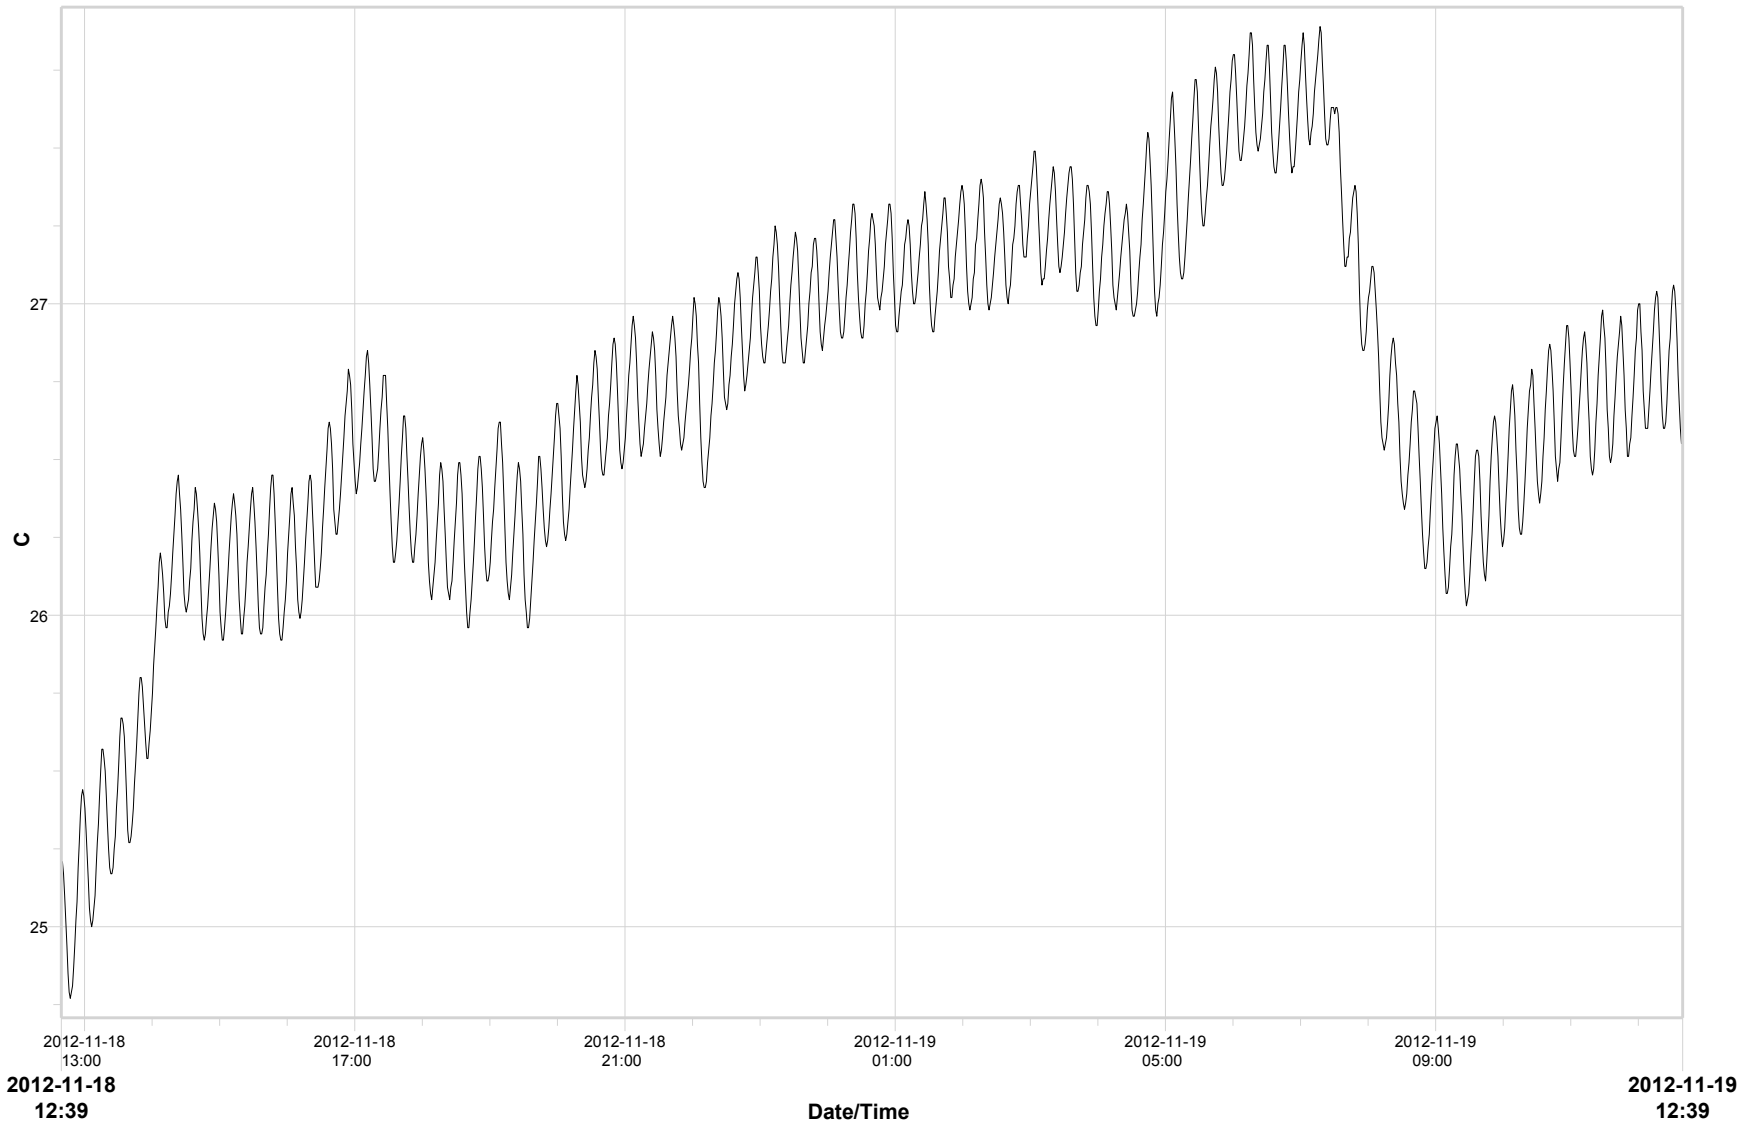

Report Summary Statistics

#	Location	Zone	Color	Units	Avg	Min	Max
1	Temperature (43918)	System/Zone P (43905)	■	C	26.71	24.77	27.89

Report Summary Statistics

#	Location	Zone	Color	Units	Avg	Min	Max
2	Humidity (43916)	System/Zone P (43905)	█	RH	31.3	26.3	38.0

Summary for C locations

#	1
Plot Legend:	█
Location:	Temperature (43918)
Zone:	System/Zone P (43905)
Units:	C
Device Serial Number:	11021095
Hardware Model:	2000 VL
Hardware Revision:	3.57
Firmware Version:	3.2-B5
Security:	Secure
Last Calibrated By:	Vaisala Canada Inc
Last Calibration Date:	2012-02-01
Next Calibration Date:	2013-02-01
Host:	viewlincServer